


North Carolina State Hearing Aid Dealers and Fitters Board

Practice Simulation: 1

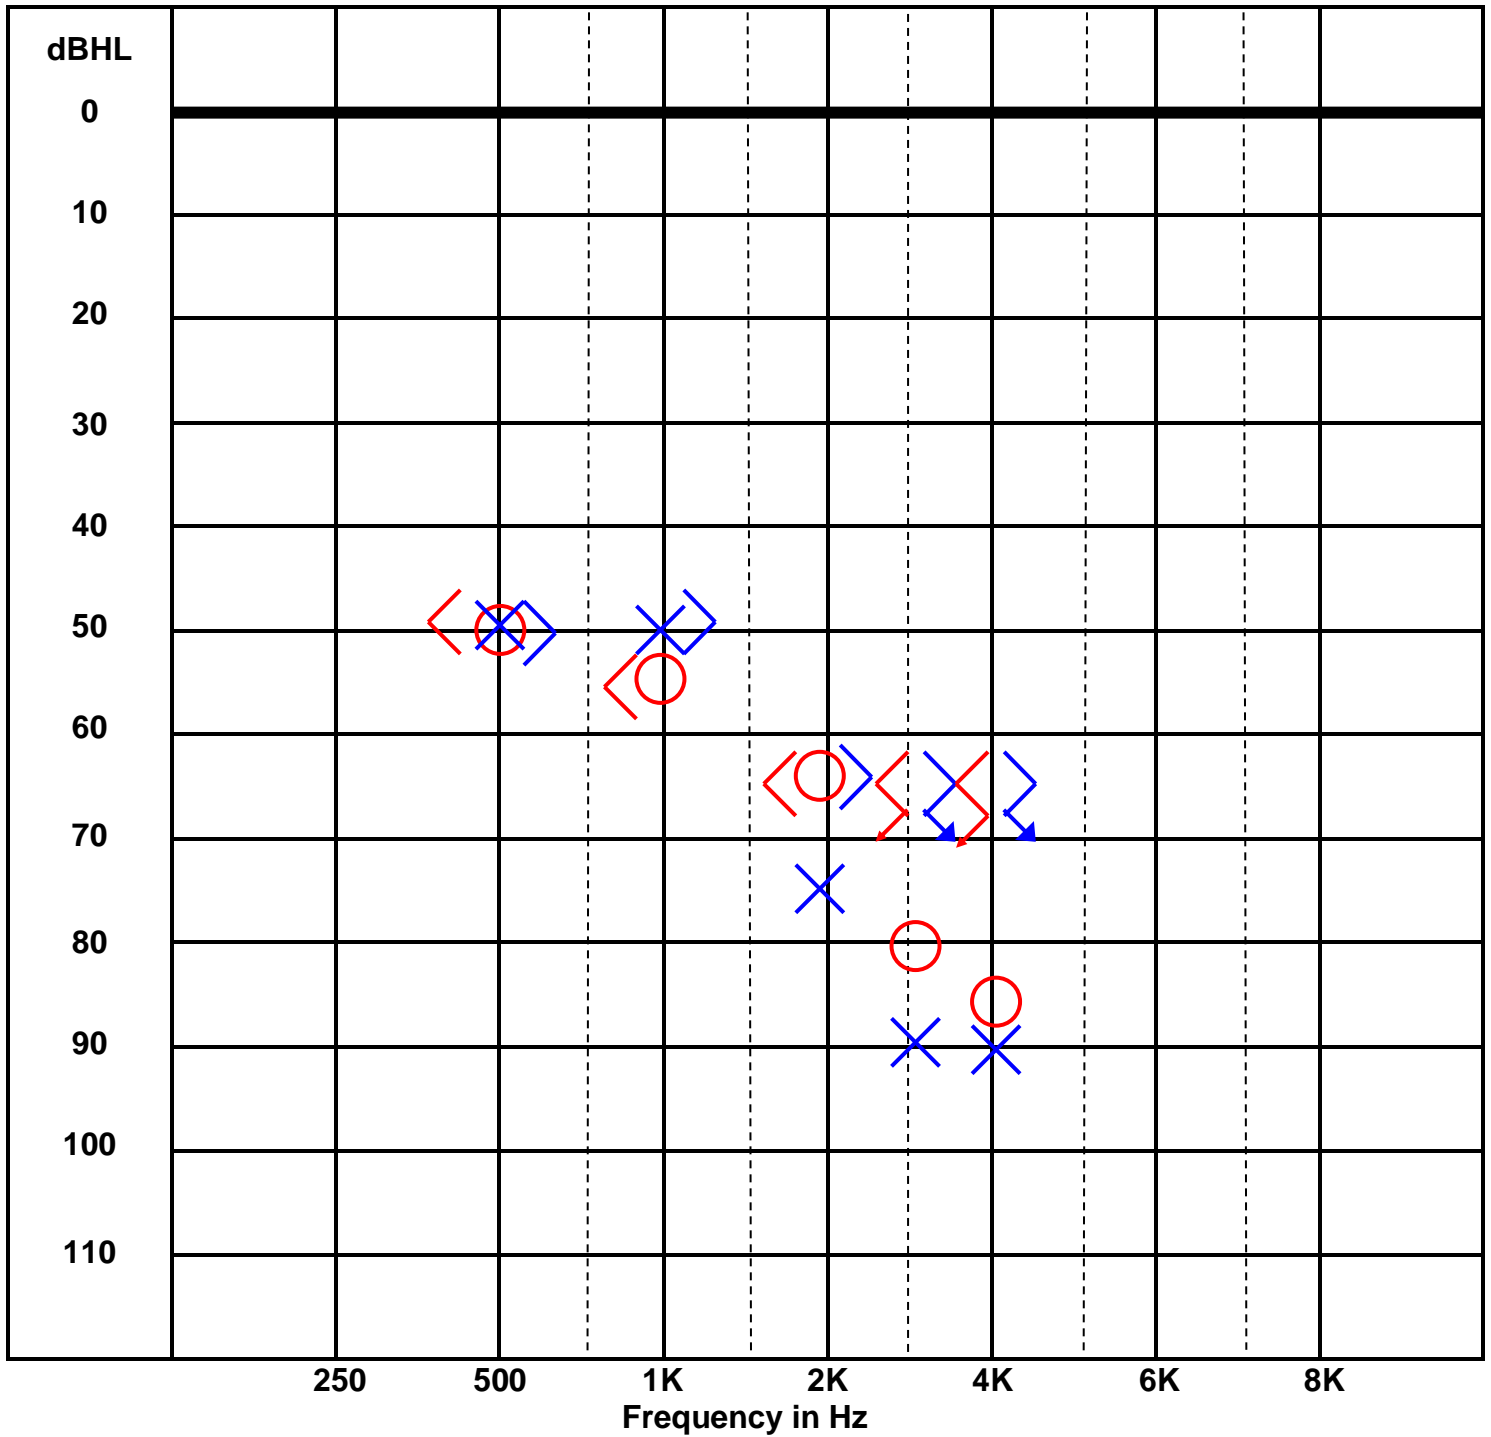

Maximum Limits
Air Conduction = 110 dBHL
Bone Conduction = 65 dBHL