


# North Carolina State Hearing Aid Dealers and Fitters Board

## Practice Simulation Key: 3

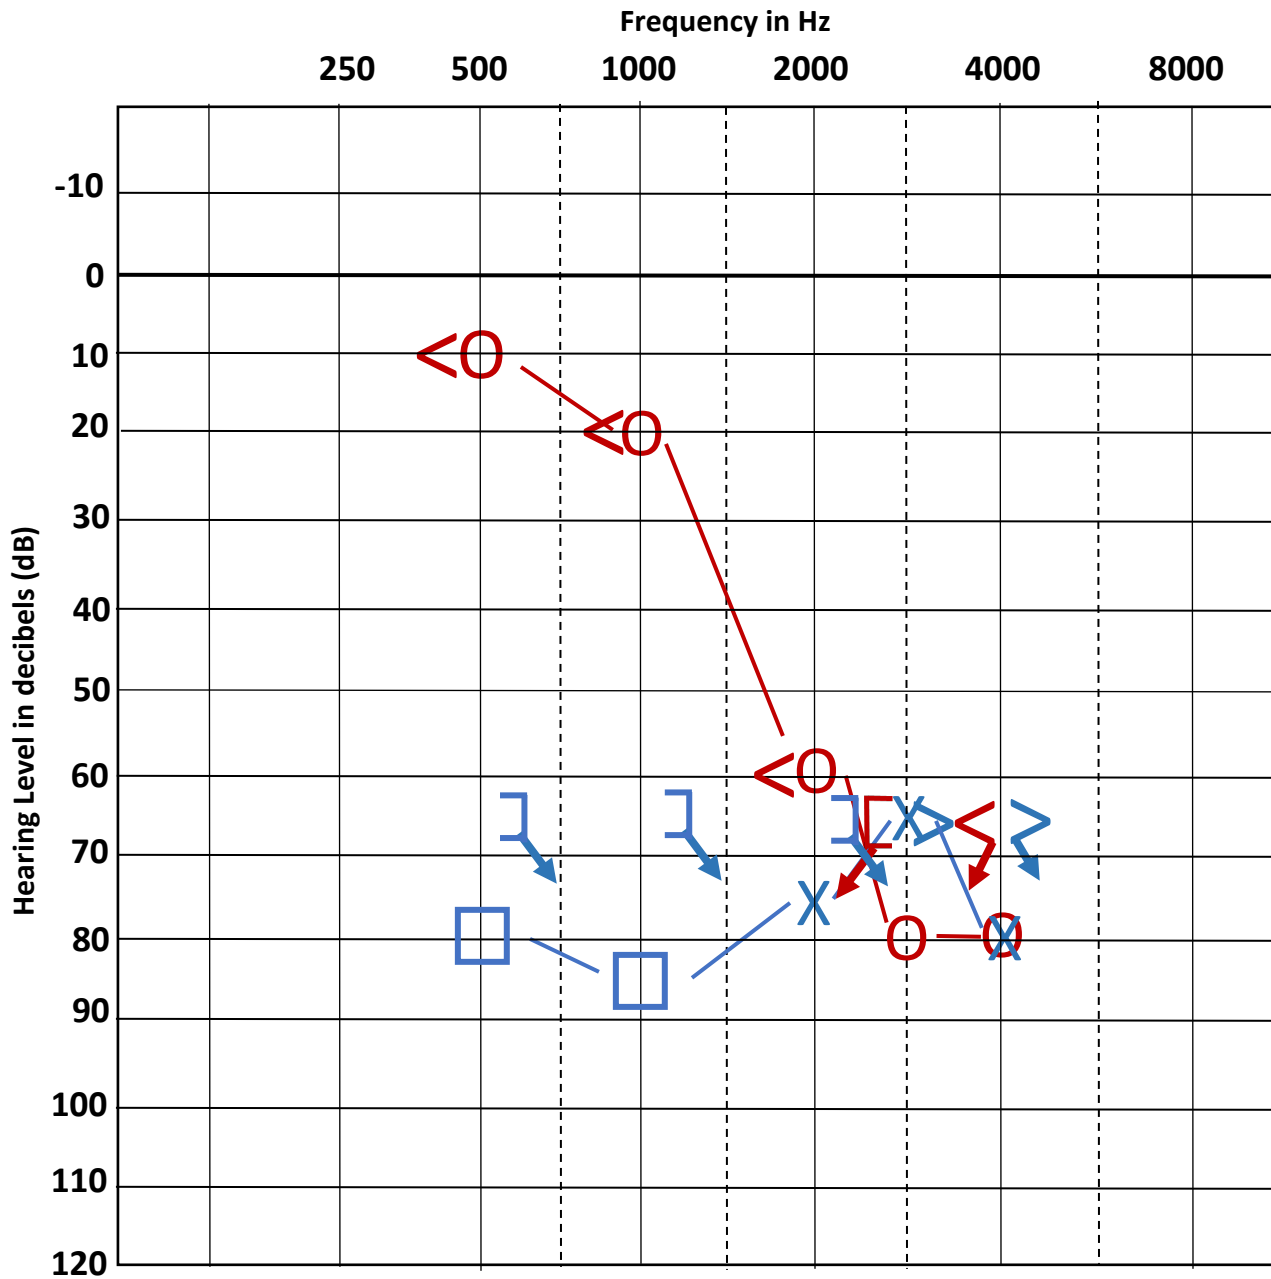

Maximum Limits:  
Air Conduction: 110 dBHL  
Bone Conduction: 65 dBHL