


North Carolina State Hearing Aid Dealers and Fitters Board

Practice Simulation Key: 2

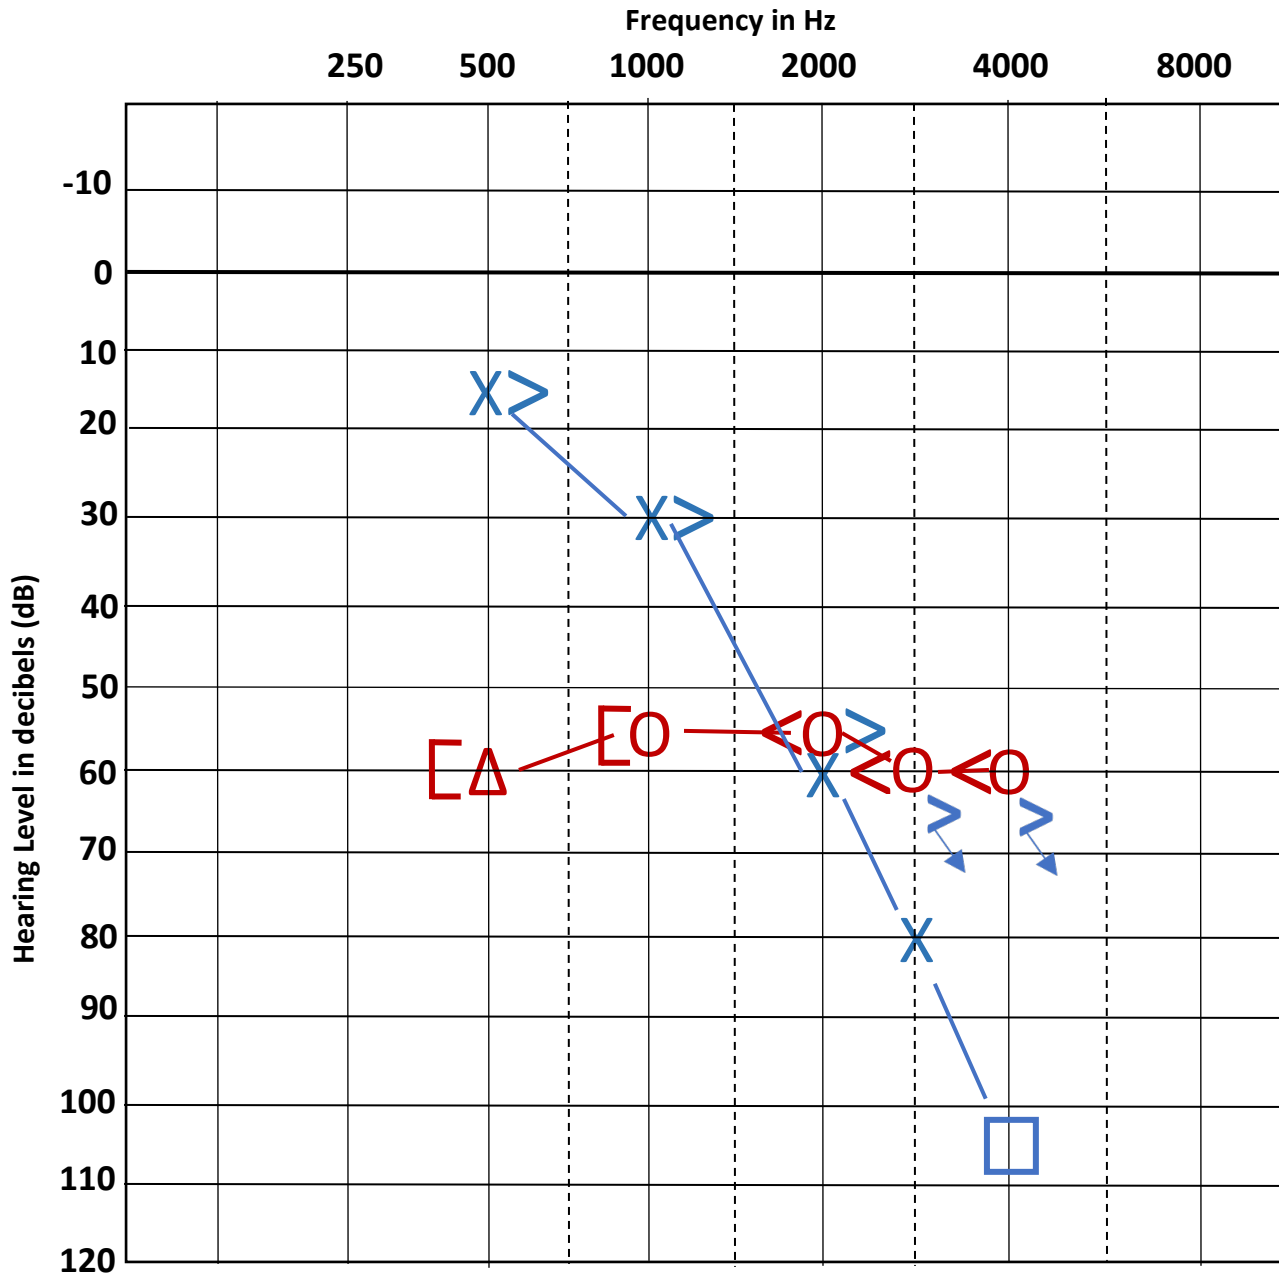

Maximum Limits:

Air Conduction: 110 dBHL

Bone Conduction: 65 dBHL